

# An Automatic Fall Detection Framework Using Data Fusion of Doppler Radar and Motion Sensor Network

Liang Liu, *Student Member, IEEE*, Mihail Popescu, *Senior Member, IEEE*, Marjorie Skubic, *Senior Member, IEEE*, Marilyn Rantz, *Member, IEEE*

**Abstract**— This paper describes the ongoing work of detecting falls in independent living senior apartments. We have developed a fall detection system with Doppler radar sensor and implemented ceiling radar in real senior apartments. However, the detection accuracy on real world data is affected by false alarms inherent in the real living environment, such as motions from visitors. To solve this issue, this paper proposes an improved framework by fusing the Doppler radar sensor result with a motion sensor network. As a result, performance is significantly improved after the data fusion by discarding the false alarms generated by visitors. The improvement of this new method is tested on one week of continuous data from an actual elderly person who frequently falls while living in her senior home.

## I. INTRODUCTION

In the USA, falling increases the risk of death among elders above the age of 65. Over the past decade, the death rate triggered by falls among seniors is growing quickly [1-3]. The positive outcome closely relates to the fast response and medical intervention from the informed nursing personnel after the occurrence of a fall [4].

It has been reported that 90 percent of adults over the age 65 prefer to stay in their residence as they age [5]. With the new research trend on technologies, “aging in place” enables the senior to live at home independently as long as possible. The interdisciplinary researchers from the University of Missouri [6] have developed noninvasive technologies to support a local community aging in place, Tiger Place. Research from this community has promising results, including studies with smart carpet, video camera, depth image, infrared cameras and microphone arrays [7-11]. Among those technologies, the automatic fall detection system provides those in independent living with a possible alert system with a lower healthcare costs [12]. Some of the researchers have focused on the fall detection system with the visual based system and obtained good results, even under some extreme situations, such as light changing, furniture occlusion, etc. However, resident privacy may be

an issue to overcome. The visual system could not report a lethal fall if the fall occurs in the bedroom, bathroom or closet, where the residents are reluctant to be visually monitored.

The motion based system addresses the concern about privacy protection and wider detection range coverage. One example of motion sensor implementation is the Doppler radar. The Doppler radar can sense, track, and recognize moving objects and surveillance human activity. It has been successfully applied to extract velocity and stride length for measuring gait parameters in [13-15]. The Doppler radar can detect falls by producing specific signatures for various part of falling human body. The previous works have shown encouraging performance of the fall detection system with Doppler radar (\$50/radar unit) in laboratory with different radar sensor displacement [16-18].

Another example is the passive infrared sensor (PIR) motion sensor network that has been used at TigerPlace since 2005. It reports the absent or present of the resident at a certain location in the home. Its application concentrates on the life style pattern of seniors to tell the physical and cognitive health conditions and find the deviate from the norm pattern [19]. The older adult activity pattern is represented with an activity density map. The map computes the density  $d$  with the number of all motion hits  $s$  during an hour divided by time at home during that hour  $t$ , which is  $d=s/t$ . If there is a continuous motion detected, sensors will generate an event in every 7 second.

In this paper, an improved fall detection framework is proposed by fusing the radar sensor and the PIR motion sensor networks in the home of an older adult, who is an actual faller. As the conclusion in [18], the radar sensor is placed on the ceiling for a better detection. We also propose different data fusion schema to eliminate possible false alarms. The paper is organized as follows. Section II introduces the methodology. We present results in section III and give conclusion and ongoing work in section IV.

## II. METHODOLOGY

Our aim is to detect falls of the elderly resident with higher accuracy, especially for the case when the resident is alone. The Doppler radar sensor is sensitive to motion mainly when there are visitors in the apartment, such as repairman, housekeeper, family, friends, *etc.* Those high energy activities add noise to the resident’s activity data and generate false alarms in the fall detection algorithm.

This project was supported by grant R01HS018477 from the Agency for Healthcare Research and Quality (AHRQ). The content is solely the responsibility of the authors and does not necessarily represent the official views of the AHRQ.

Liang Liu and Marjorie Skubic are with the Electrical and Computer Engineering Department, University of Missouri, Columbia, MO 65211 USA (e-mail: llpfd@mail.missouri.edu, SkubicM@missouri.edu).

Mihail Popescu is with the Health Management and informatics Department, University of Missouri, Columbia, MO 65211 USA (e-mail: PopescuM@missouri.edu).

Marilyn Rantz is with the Sinclair School of Nursing, University of Missouri, Columbia, MO 65211 USA (e-mail: RantzM@health.missouri.edu).

### A. Motion sensors placement in the home environment

We have deployed ceiling radars in six different apartments in Tiger Place. The typical floor plan of a TigerPlace apartment is shown in figure 1. There are seven motion sensors (located at the end of each cone of blue lines) and one Doppler radar facing down to the floor (marked by a red cross in figure 1) placed above the ceiling at the center of the living room and dining room. The detection range of the radar is about 6 and the height of the room is about 3 m. The data logger for each sensor is synchronized with the same data server in Tiger Place.

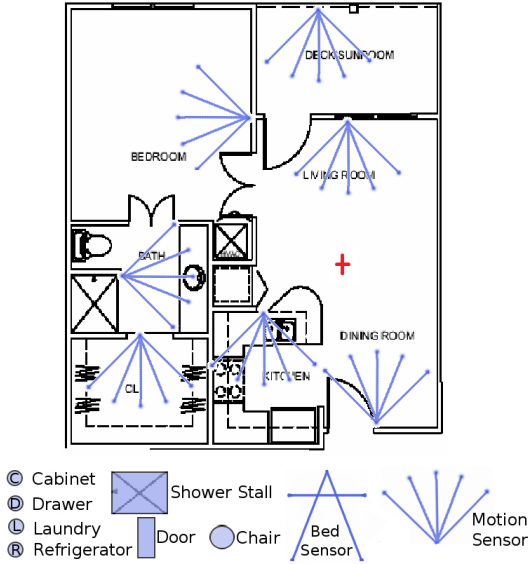


Fig. 1. The floor plan with motion sensors placement in a senior apartment.

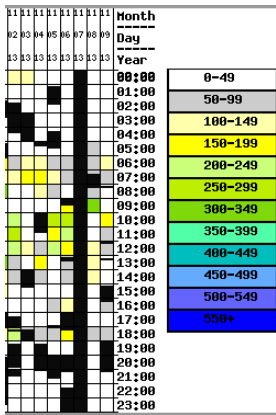


Fig. 2. Activity density map.

### B. Activity density map generated by the sensor network

In the resident activity density map shown in figure 2, the x-axis represents days from left to right and y-axis denotes hours in a day. Each color represents the different motion density levels. The black on density map means that the resident is away from home. The white represents very low density. The color bar illustrates the density range from 50~99 events/h to >550 events/h using different color blocks from gray to blue sequentially.

### C. Description of Doppler radar sensor features

For the Doppler radar sensor signal segment  $r(n)$ , we first take the short time Fourier transform (STFT) by

$$STFT(m, \omega) = \sum_{n=-\infty}^{\infty} r(n)w(n-m)e^{-i\omega n}. \quad (1)$$

Then, we compute the spectrogram by taking the magnitude square to the STFT,

$$spectrogram\{r(n)\} \equiv |STFT(m, \omega)|^2. \quad (2)$$

Next, we calculate the energy burst curve using

$$EB(m) = \sum_{\omega=25/(2\pi)}^{50/(2\pi)} STFT(m, \omega), \quad (3)$$

and smooth the curve over K bursts to reduce noise:

$$\bar{EB}(m) = \sum_{i=0}^{K-1} EB(m-i). \quad (4)$$

The peaks on this curve are the located potential falls. More detailed examples are presented in [18].

We extract MFCC features for each 2-second window which contains the located possible fall activities. Each of the 2-second window data segment is divided into 166 sub-frames with an overlap rate of 0.5. Seven coefficients are extracted from each sub-frame. After throwing the dominant coefficient away, we use  $6 \times 166 = 996$  MFCC features to represent this potential fall.

The radar signatures are classified by support vector machine (SVM) into two classes: fall and non falls. We employed LibSVM [18] to produce a score, fall confidence  $conf_{fall}$ . For computational efficiency, we used only a linear kernel for SVM in all our experiment. We generate a receiver operating characteristic (ROC) curve by thresholding the SVM scores to evaluate the performance of our fall detection algorithms.

### D. Data fusion schema

The output from above Doppler radar system are in the form of a radar fall confidence  $conf_{fall}$  associated with the corresponding time stamp  $t_{radar}$ . The sensors in the motion sensor networks are installed above the door of each room and the main facility area, such as kitchen, bathroom, and closet. An event from the motion sensor network means someone is moving around the sensor. A fall is unlikely to occur if an event from a motion sensor is recorded immediately after it. Figure 3 illustrates the idea of this assumption. The  $t_{dist}$  represents the time lapse between  $t_{radar}$  and the afterwards closest event time stamp  $t_{motion}$ . It is defined as  $t_{dist} = t_{motion} - t_{radar}$ .

A predefined parameter  $\Delta$  is used to determine whether the  $t_{dist}$  is among the reasonable range for a real fall. If the time lapse is shorter than  $\Delta$ , it is a false alarm. Otherwise, it is a fall. The rule is represented by

$$\begin{cases} \text{if } t_{dist} < \Delta, & \text{false alarm} \\ \text{if } t_{dist} \geq \Delta, & \text{fall} \end{cases} \quad (5)$$

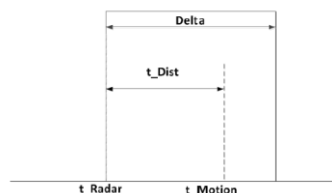


Fig. 3. Data fusion schema between Doppler radar and sensor network.

E. Description of data collected by ceiling radar

The experimental data includes training data from stunt actors and the continuous testing data from the elderly adult home. Due to the large dataset and limited space, only one week’s data from an actual elderly person who frequently falls are presented in this paper.

The dataset in Table I was collected with ceiling radar at senior apartments in TigerPlace. The stunt actor came to senior apartments monthly to perform different types of falls and non-falls. The falls performed were 21 types including lose balance, lose consciousness, trip & fall, reach & fall in different directions - forward, backwards, left side, right side falls, and fall from couch. Non-falls were also collected of daily activities that could be easily confused with fall activities and cause false alarms in fall recognition, such as bending down to pick up from floor, drop stuff on the floor, sit down on floor, kneel down to tighten the shoe, etc.

TABLE I. STUNT ACTOR DATASET

Environment	Fall #	Non-fall #
Tiger Place	72	98

III. EXPERIMENTAL RESULTS

A. Improving the performance by including the sensor network

In figure 4, the blue solid line gives the fall confidence generated by Doppler radar fall detection system. The red dotted line presents the event activated by the sensor network. The x-axis denotes the timestamp for both of the sensor system.

Figure 4 (a) shows that a fall is recognized by the radar with a confidence 0.96. No event is reported from the sensor network in the following 55 seconds. Figure 4 (b) presents the typical false alarms from the senior daily activities: fast opening and closing the door near to ceiling radar (0.98 fall confidence); fast turning around and shifting the walker direction (0.83 fall confidence). Multiple events from sensor network after Non-fall-2 reflect that the resident is active or a visitor is in the apartment. Although the motion is not frequent after Non-fall-2, this false alarm can be still removed with a larger *Delta* value.

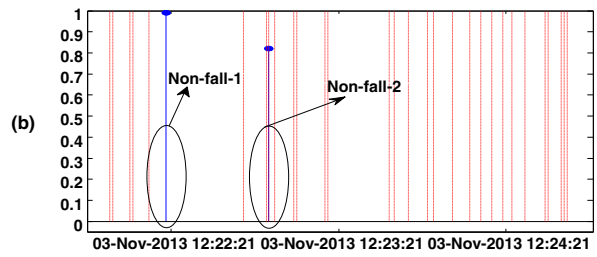
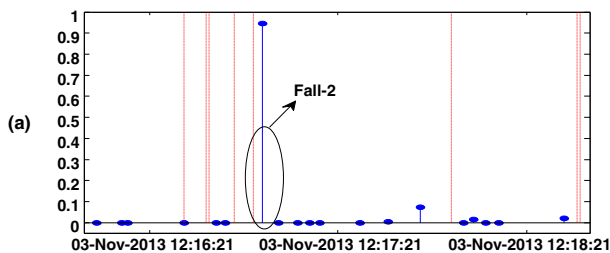


Fig. 4. The examples fall confidence with events from the sensor network: (a) a natural fall (top); (b) non-fall (bottom).

B. Leave-one-out cross validation for the stunt actor dataset collected with ceiling Doppler radar sensor

The leave-one-out cross validation is applied on the stunt actor data in Table I. For N=170 samples, each experiment of this validation uses N-1 samples for training and the rest sample for testing. In figure 5 we show the classification results of the radar signature library (see Table I) where we achieved an area under the ROC curve (AUC) of 0.98. While good results were obtained on the signature library, we couldn’t replicate them on the continuous datasets.

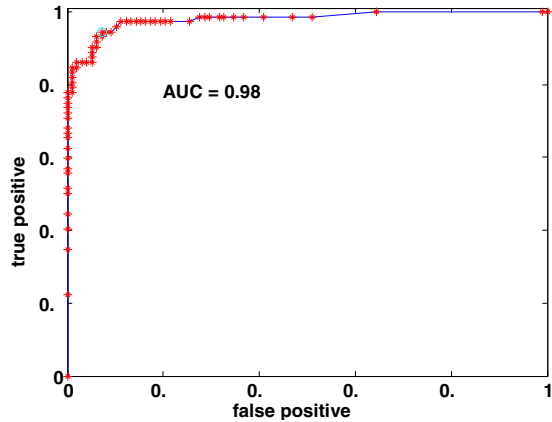


Fig. 5. The cross validation of the stunt actor dataset.

C. Data fusion results for the actual faller

Using the above stunt actor data for training, we tested our fusion method on one week of continuous data collected in a TigerPlace apartment. In figure 6, the false alarm number reduces 63% false alarm while the parameter *Delta* is increasing from 0 to 53 seconds (from right to left). Without the motion sensor network, the fall detection system generates 172 false alarms per day in order to detect all the actual falls. The best performance of the improved system could achieve 62 false alarms per day without losing any falls when *Delta* equals to 53 seconds. If the *Delta* is larger than 53 second, the false alarm keeps decreasing but there will be some missing falls.

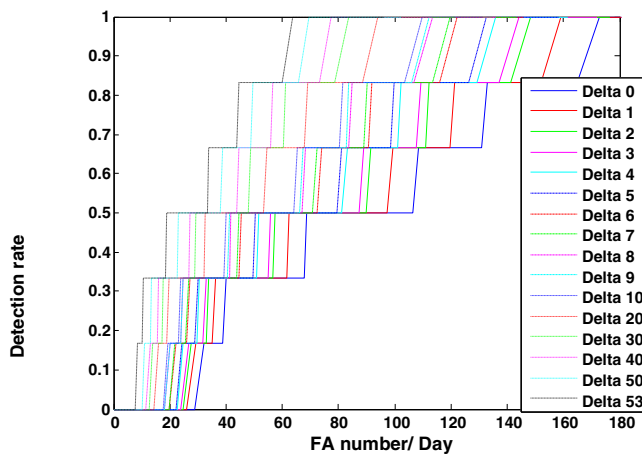


Fig. 6. The performance of the improved fall detection system on one week elderly home data.

It is reasonable to choose the best *Delta* value as about 50 seconds. An actual elderly faller could not probably get up by herself to activate the sensor network within 50 seconds after a fall occurs. If any event is generated within 50 seconds, the detected possible fall is most likely to be a false alarm and will be discarded. The remaining fall confidence is kept to generate the ROC curve as seen in figure 6. We did not consider the case that the elderly adult had a real fall and a visitor was there to generate events in the sensor network. In this case we assume that visitor would help the person who fell or call a staff member.

In Table II, four falls are detected with a higher fall confidence ( $>0.9$ ). The fall-1 and fall-4 generate a lower confidence ( $<0.5$ ) due to the weak radar signals. The fall-1 is around at the detection range of the ceiling radar. The fall-4 is a kind of slow motion style fall, for which we assume the resident usually would not get a fatal injury. By applying the sensor network fusion framework, we could detect all those natural elderly falls by generating a lower false alarm number (even the fall confidence is small).

TABLE II. DESCRIPTION DETECTED RESIDENT FALLS IN A WEEK

# Fall	Fall and accompanying activities (observed with Kinect depth image)
1	close front door
2	resident kneeled first, then fell to the side
3	visitor behind kitchen counter, cat run
4	kneeled first fall, sit on leg and fall
5	one leg kneel first
6	sliding away the wheel chair and fall

#### IV. CONCLUSIONS

This paper proposes an improved fall detection framework that uses the fusion between a Doppler radar system and a motion sensor network. We tested our method on a pilot dataset obtained in an apartment in TigerPlace. Using our framework we reduced the false alarm rate by 63% on one week of continuous data including six natural falls.

Our further goal will focus on improving the performance of monitoring the elderly fall in a longer term (more data).

#### ACKNOWLEDGMENTS

This work was supported in part by the Agency for Healthcare Research and Quality under grant R01-HS018477 (Rantz, PI). The content is solely the responsibility of the authors and does not necessarily represent the official views of the Agency for Healthcare Research and Quality.

#### REFERENCES

- [1] Murhy SL, "Deaths: Final Data for 1998," *National Vital Statistics Reports*, vol. 48, no. 11. Hyattsville, Maryland: NCHS, 2000.
- [2] Centers for Disease Control and Prevention, National Center for Injury Prevention and Control. *Web-based Injury Statistics Query and Reporting System (WISQARS)* [online]. Access November 30, 2010
- [3] Stevens JA. Fatalities and injuries from falls among older adults – United States, 1993–2003 and 2001–2005. *MMWR* 2006a;55(45).
- [4] C. G. Moran, R.T. Wenn, M. Sikand, A.M. Taylor, Early mortality after hip fracture: is delay before surgery important", *J. of Bone and Joint Surgery*, pp. 483-9, 2005.
- [5] "A Report to the National Livable Communities: Creating Environments for Successful Aging"[online]. Retrieved 2014-03-10.
- [6] M. Rantz, M. Aud, G. Alexander, B. Wakefield, M. Skubic, R.H. Luke, D. Anderson, and J. Keller, "Falls, technology, and stunt actors: new approaches to fall detection and fall risk assessment," *Journal of Nursing Care Quality*, vol. 23(3), pp. 195-201, 2008.
- [7] Stone E & Skubic M, "Unobtrusive, Continuous, In-HomeGait Measurement Using the Microsoft Kinect," *IEEE Transactions on Biomedical Engineering*, 2013, 60(10):2925-2932.
- [8] A. Sixsmith, N. Johnson, R. Whatmore, "Pyrolytic IR sensor arrays for fall detection in the older population", *J. Phys. IV France*, vol. 128.
- [9] M. Addlesee, A. Jones, F. Livesey, and F. Samaria, "the ORL active floor," in *IEEE Personal Communications*, vol. 4.5, 1997, pp. 35-41.
- [10] Li Y, Banerjee T, Popescu M & Skubic M, "Improvement of Acoustic Fall Detection using Kinect Depth Sensing," *Proceedings, IEEE 2013 International Conference of the Engineering in Medicine and Biology Society (EMBC)*, Osaka, Japan, July 3-7, 2013.
- [11] Wang F, Stone E, Skubic M, Keller JM & Abbott C, "Toward a Passive Low-Cost In-Home Gait Assessment System for Older Adults," *IEEE Journal of Biomed. Health Inf.*, 2013, 17(2):346-355.
- [12] Demiris G, Rantz MJ, Aud MA, Marek KD, Tyrer HW, Skubic M & Hussam AA, "Older Adults' Attitudes Towards and Perceptions of 'Smarthome' Technologies: a Pilot Study," *Medical Informatics and The Internet in Medicine*, June, 2004, vol. 29, no. 2, pp. 87-94.
- [13] M. Otero, "Application of a continous wave radar for human gait recognition," *The MITRE Corporation*, 2005.
- [14] Yardibi T, Cuddihy P, Genç S, Buñi C, Skubic M, Rantz M, Liu L, Phillips C, "Gait characterization via pulse-Doppler radar," *IEEE International Pervasive Health*, pp.662-667, March 21-25, 2011
- [15] Cuddihy PE, Yardibi T, *etc*, "Radar Walking Speed Measurements of Seniors in their Apartments: Technology for Fall Prevention," 34th Annual International Conference of the IEEE Engineering in Medicine and Biology Society, pp 260-263, Aug 28-Sep 1, 2012.
- [16] Liu L, Popescu M, Skubic M, Rantz M, Yardibi T & Cuddihy P, "Automatic Fall Detection Based on Doppler Radar Motion," *Proceedings, 5th International Conference on Pervasive Computing Technologies for Healthcare*, Dublin, Ireland, May 23-26, 2011.
- [17] Liu L, Popescu M, Rantz M, Skubic, "Fall Detection using Doppler Radar and Classifier Fusion," *Proceedings of EMBS on BHI*, Shenzhen, Jan 2-7, 2012.
- [18] Liu L, Popescu M, Ho KC, Skubic M & Rantz M, "Doppler Radar Sensor Positioning in a Fall Detection System," 34th Annual International Conference of the IEEE Engineering in Medicine and Biology Society, pp 256-259, Aug 28 - Sep 1, 2012.
- [19] Wang S, Skubic M & Zhu Y, "Activity Density Map Visualization and Dis-similarity Comparison for Eldercare Monitoring," *IEEE Journal of Biomedical and Health Informatics*, 2012, 16(4):607-614.